

FIG. 1 is a cross-sectional view of a prior art device.

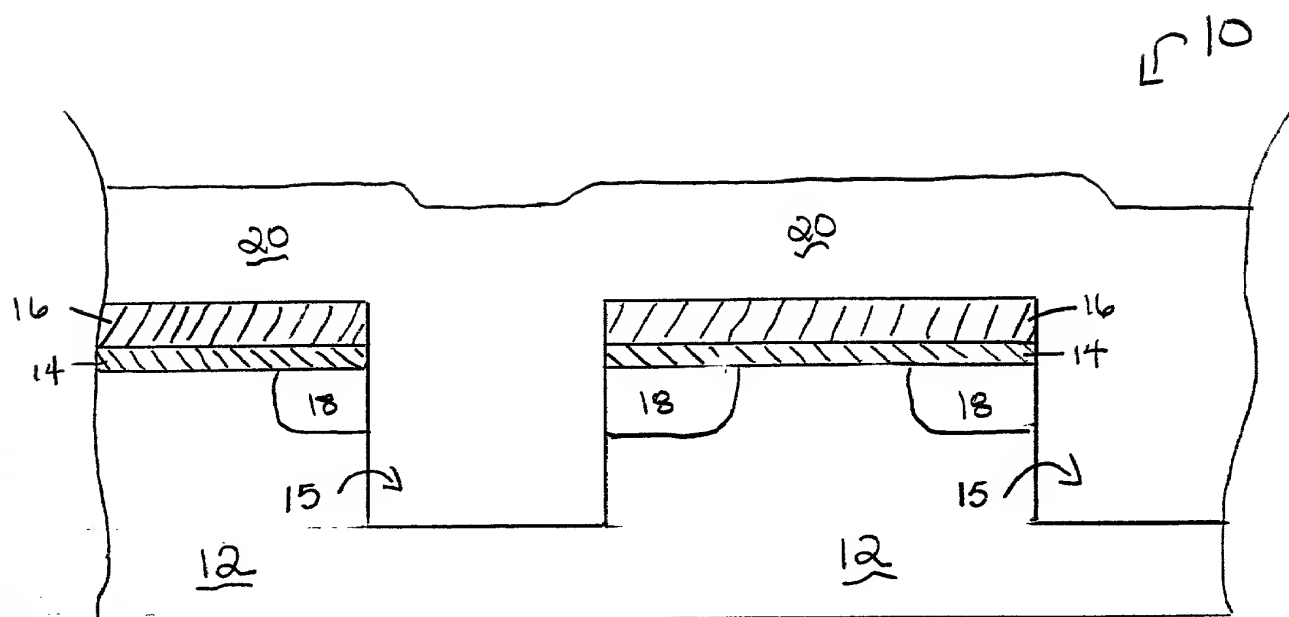


FIG. 1  
(prior art)

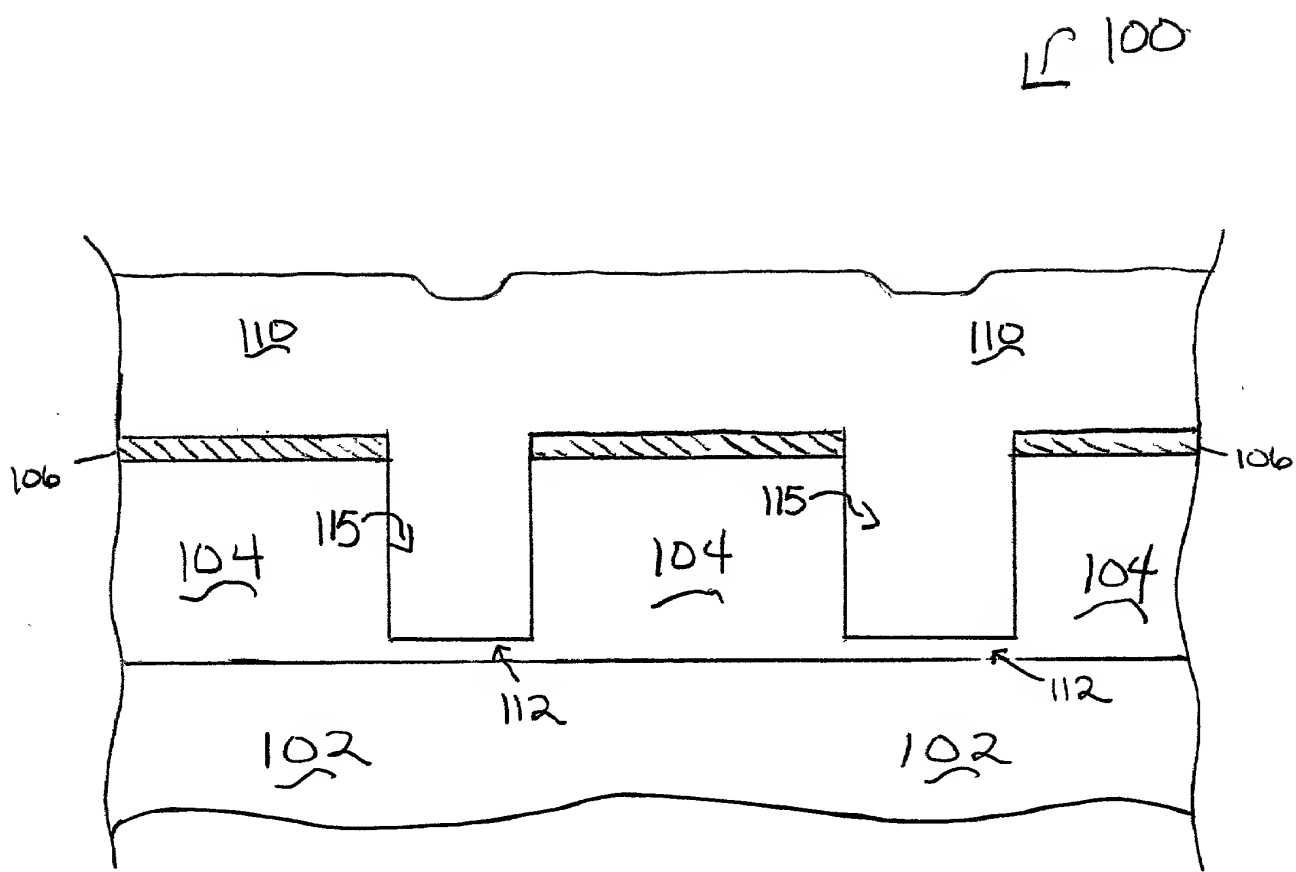


FIG. 2A

120

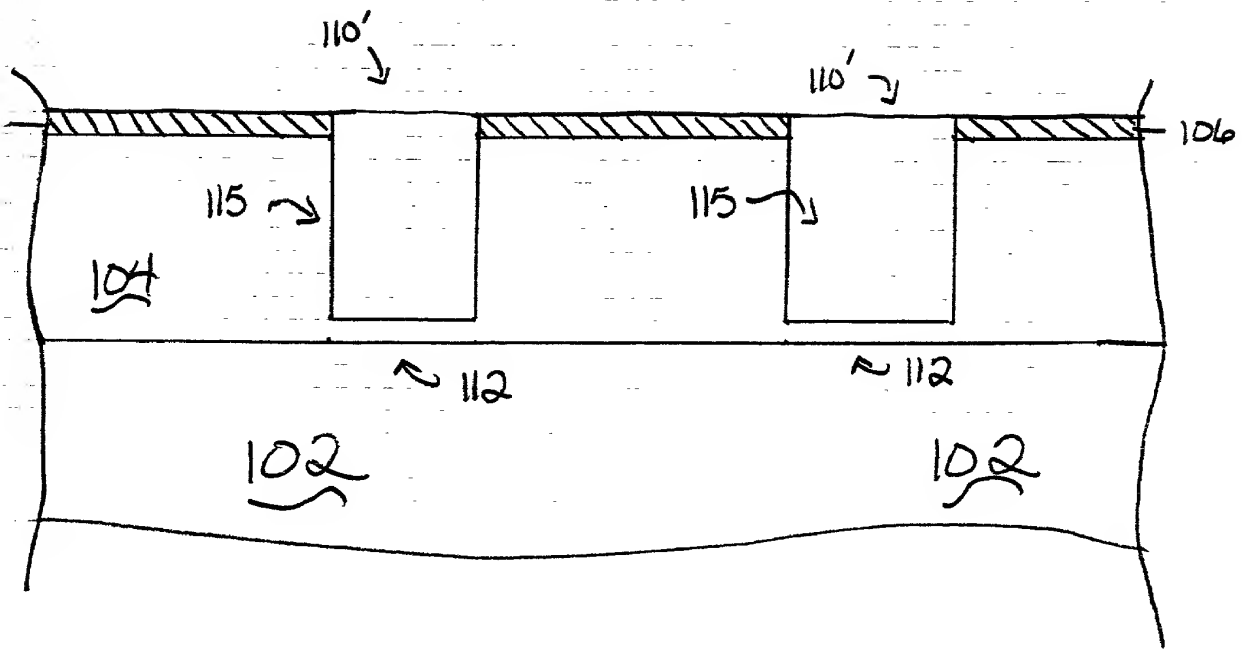


FIG 2B

130

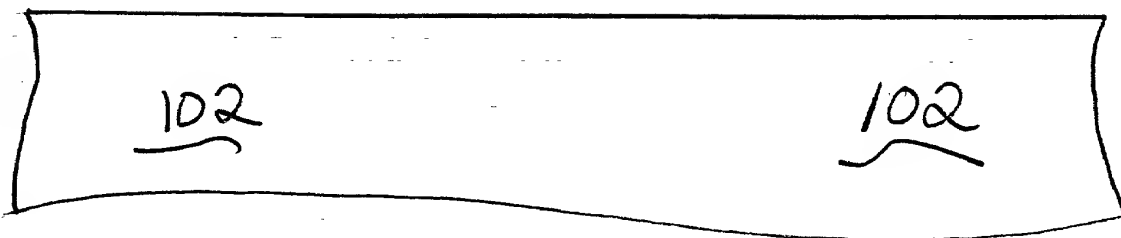


FIG 2C

140

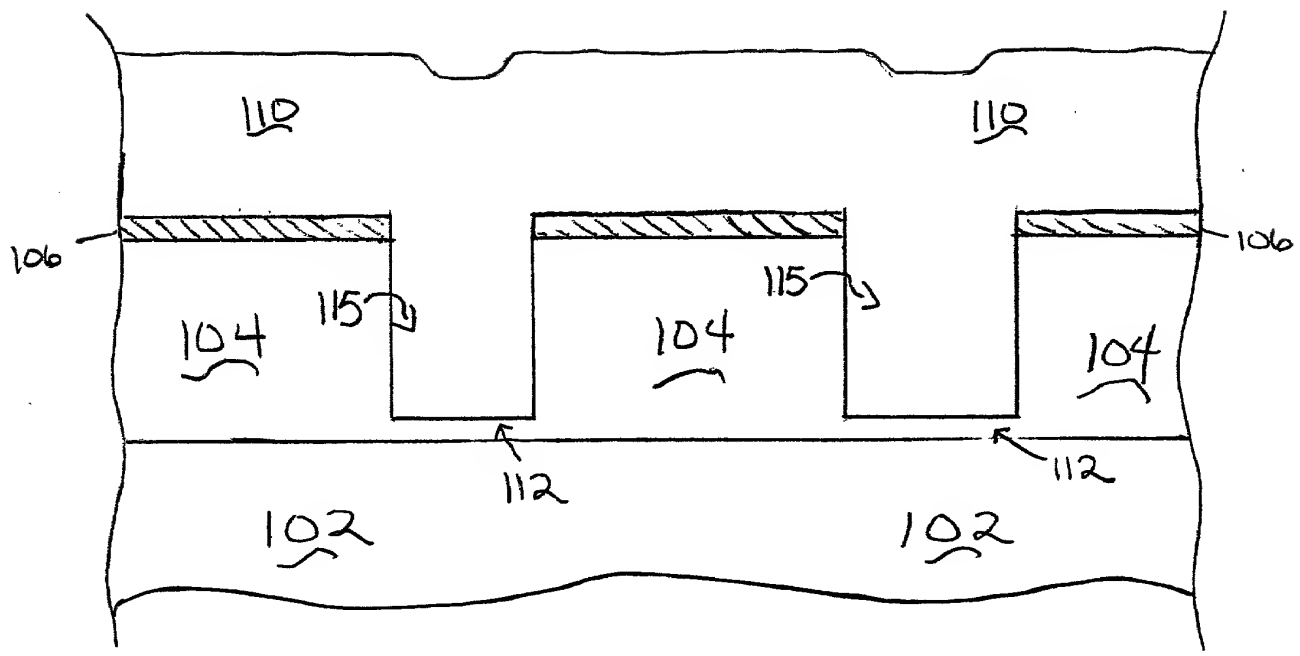


FIG. 2D

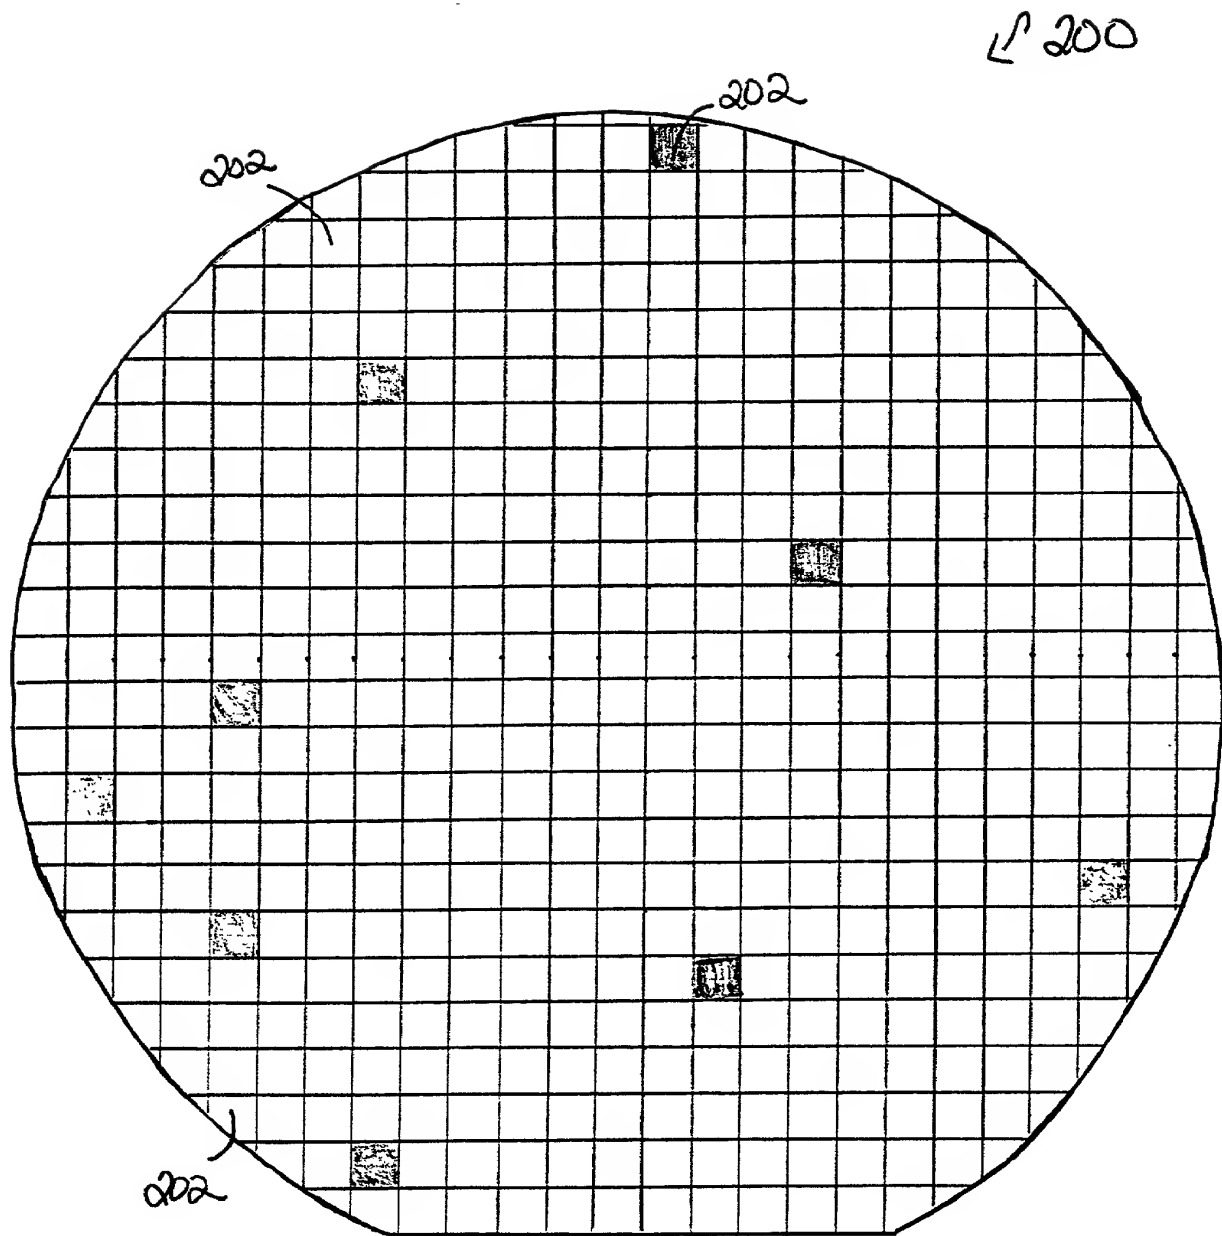


FIG. 3A

202a

204b

204c

204a

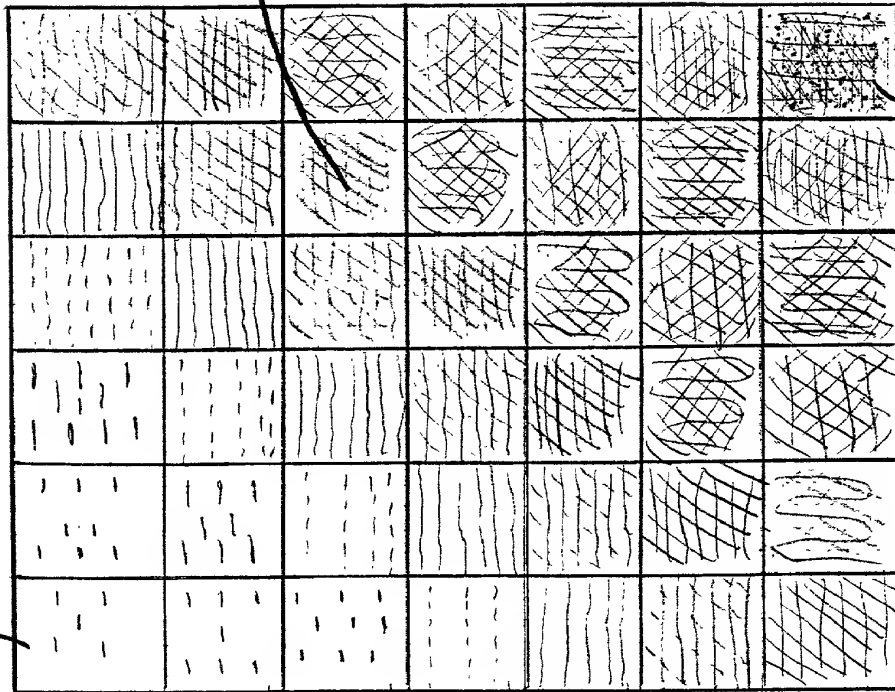


FIG. 3B

17 2025

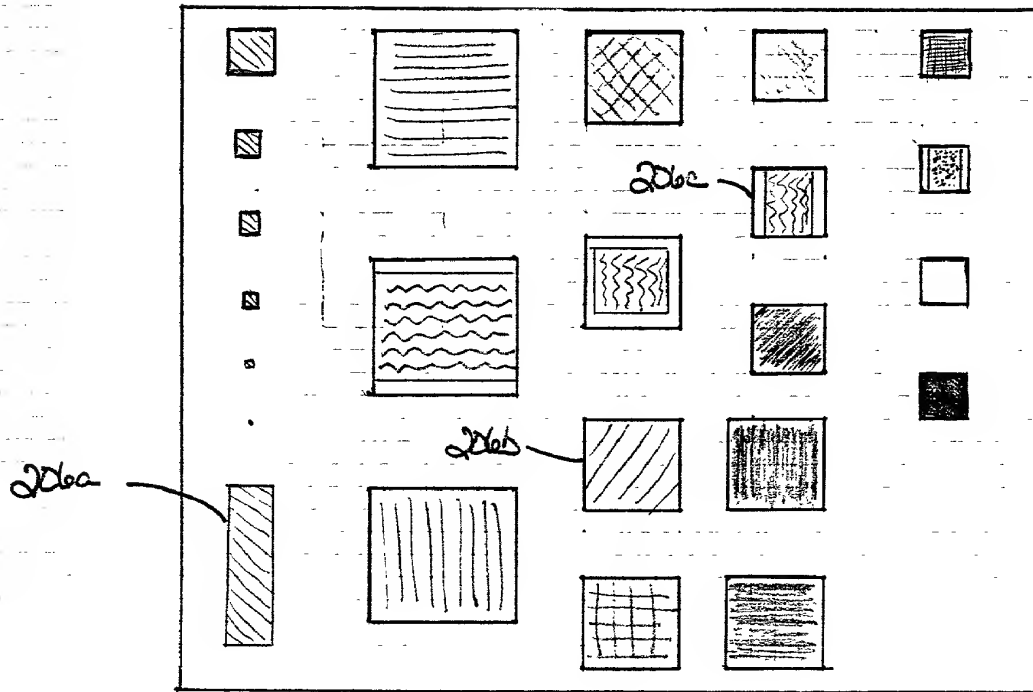


FIG. 3C



330 ↗

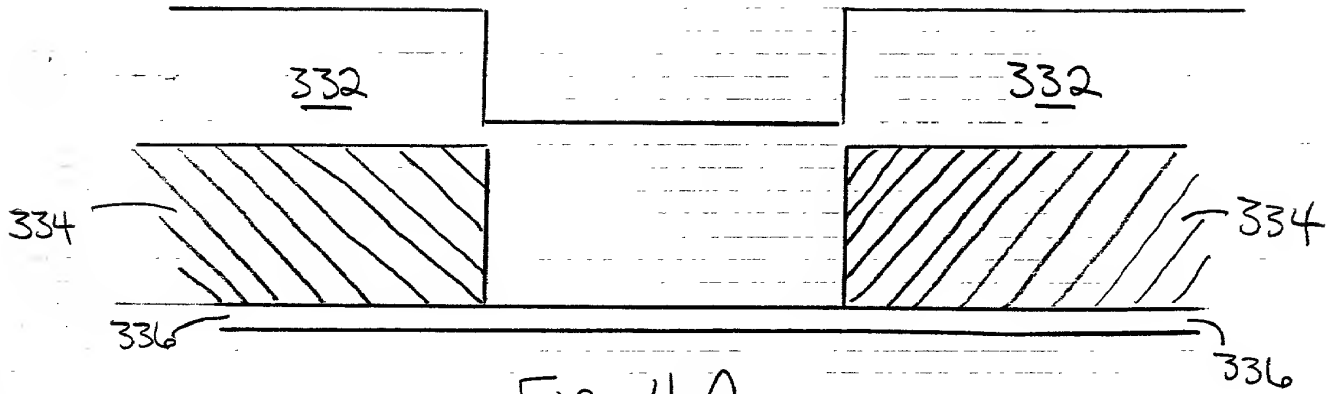


FIG 4A

340 ↗

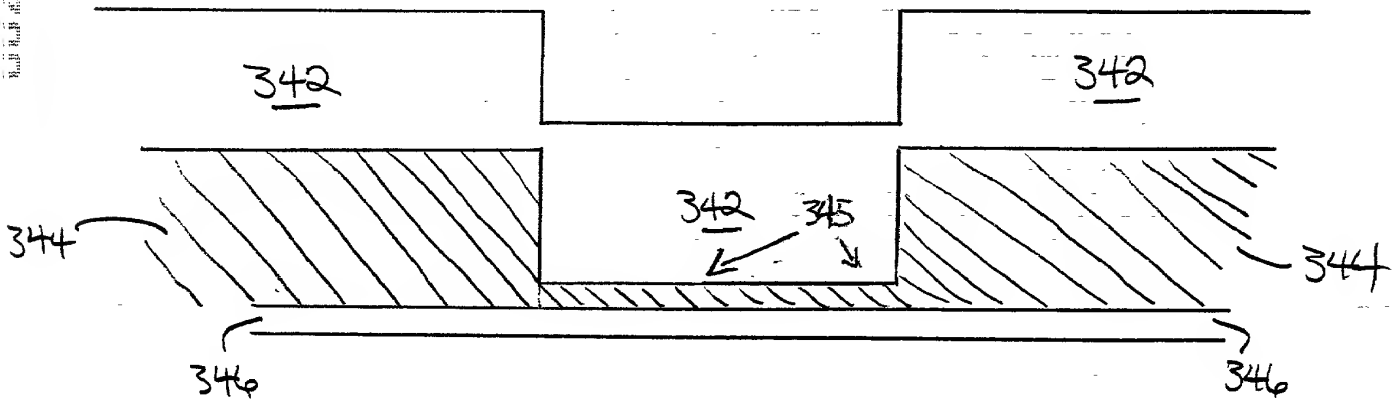


FIG 4B

300

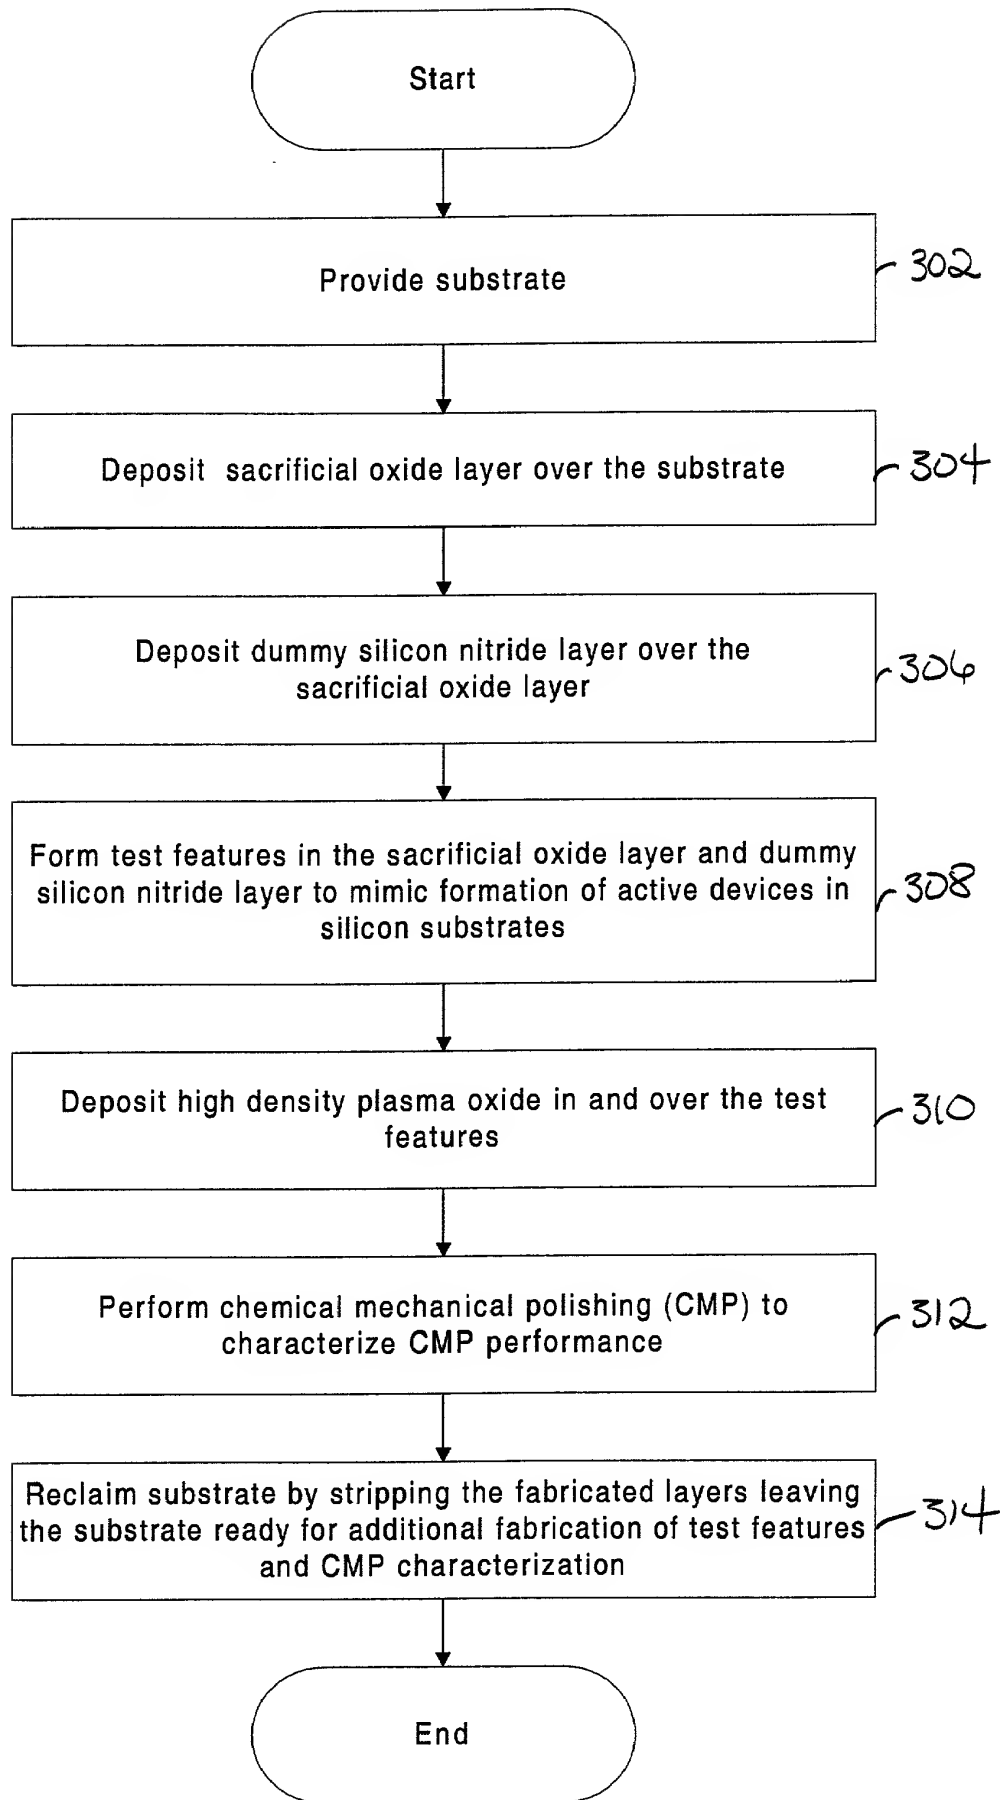


FIG 5